

Neuromuscular Response What is it and How to Measure it?

Albert Pérez-Bellmunt^{1*}, Luis Llurda¹, Mathias Simon¹, Raul Navarro¹, Oriol Casasayas¹, Carlos López-De-Celis², Roberto Seijas^{1,3} and Pedro Alavarez^{1,3}

¹Department of Basic Sciences, International University of Catalunya, Spain

²Department of Physical Therapy, International University of Catalunya, Spain

³Arthroscopy GC, Garcia Cugat Foundation Hospital Quirón, Spain

ARTICLE INFO

Received Date: June 17, 2018

Accepted Date: July 25, 2019

Published Date: July 30, 2019

KEYWORDS

Neuromuscular function
Neuromuscular response
Muscle contraction sensor
Tensiomyography
Stiffness
Myometry

Copyright: © 2019 Albert Pérez-Bellmunt et al., Physical Medicine & Rehabilitation Journal. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Citation for this article: Albert Pérez-Bellmunt, Luis Llurda, Mathias Simon, Raul Navarro, Oriol Casasayas, Carlos López-De-Celis, Roberto Seijas and Pedro Alavarez. Neuromuscular Response. What is it and How to Measure it?. Physical Medicine & Rehabilitation Journal. 2019; 2(1):118

Corresponding author:

Albert Pérez-Bellmunt,
Department of Basic Sciences,
International University of Catalunya,
Spain, Tel: +34 93 504 20 14;
Email: aperez@uic.es

ABSTRACT

The neuromuscular response or neuromuscular function is a set of biomechanical and viscoelastic properties about the muscular and fascia tissue. These characteristics are fundamental for the rehabilitation and sport medicine. This is a review of how to measure neuromuscular response and to define this concept, its parameters and present different tools (myometry and tensiomyography) to measure it.

INTRODUCTION

The Neuromuscular Response or Neuromuscular Function (NMR) is a set of biomechanical and viscoelastic properties about the myofascial tissue that prepare the muscle to perform a mechanical work as a result of muscular and nervous system function [1]. It determines the muscular performance during the movement task, its rehabilitations and its training. These parameters could be useful to assess muscle pathological or injury effects [2-4], as well as the therapeutic improvement in this tissue [5-7]. Many techniques have been used in order to measure the NMR since the mid-twentieth century, for example the Magnetic Resonance Imaging (MRI) or the Muscle Electromyography (EMG) activity. Even invasive methods have also been used in order to analyze the relationship between the contractile and histological muscle properties [8]. However, at the end of that century and the beginning of the 21st, new muscle assessment methods and tools began to be developed, such as Tensiomyography (TMG) and Myometry (MMT). Although MRI and EMG have been widely studied and lot of research has been done with these tools, few studies are available using TMG and MMT.

The aim of this review was to explain how to measure neuromuscular response and to define this concept, its parameters and newest different tools to measure it.

TENSOMYOGRAPHY

The Tensiomyography (TMG) is a tool to evaluate the muscle involuntary contractile properties and how its viscoelastic properties can influence its performance [9]. It measures parameters such as the muscle belly maximal radial displacement when it is activated by a controlled electrical stimulus [10-12]. TMG uses electrical stimulation applied percutaneously which causes a muscle contraction (Figure 1). This contraction is detected by a digital transducer applied to the muscle belly [11]. It has a good and high reliability that ranges between 0.5-2% and high reproducibility (ICC between

0.85-0.98) [13-16]. By the TMG, it can be measured the followings parameters (Figure 2 and Table 1)



Figure 1: TMG procedure.

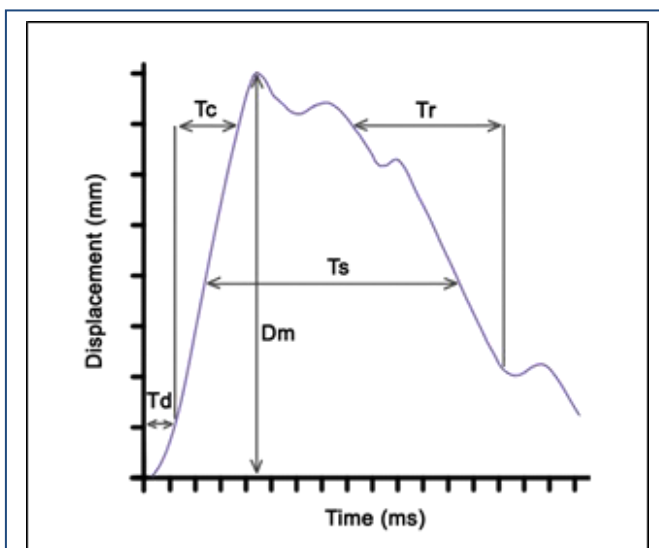


Figure 2: NMR response and TMG values.

Maximal radial Displacement (Dm)

It is the maximal radial displacement value expressed in mm. The Dm informs about muscle stiffness and it varies depending on muscle fibers disposition, volume and training. Although it is difficult to establish reference values for the Dm of the different muscles [17-19], this value tells us about the muscle tone. High values of Dm show lack of tone or fatigue; while low values show high muscle tone or stiffness [15,20,21].

Delay Time (Td)

It is measured in ms. It is the time that takes the muscle to reach from the start of the stimulus to the 10% of the total displacement of the contraction [17,19].

Contraction time (Tc)

It is measured in ms. It is the time between the 10% and 90% of the muscle displacement. Its values vary according to the muscle fiber type and fatigue [22]. Low Tc values are found in muscles with type II (white) or fast-twitch fibers predominance and high values are found in muscles with type I (red) or slow-twitch fibers predominance. The average values are usually around 28-29 ms [18] although there are authors who consider values above 30 ms as a cutoff value. The Tc is useful to distinguish athlete's types regarding their muscular qualities and to assess the workloads influence, the activation level or the fatigue during a training [139].

Sustained time (Ts): It represents the contraction sustaining time and it is measured in ms. It is the time from the 50% of the displacement reached in the contraction phase to the 50% of the displacement in the relaxation phase [17,19].

Combining all of these parameters, it is possible to obtain the **contraction velocity (Vc)**, which represents the muscle radial deformity over time. It is really useful to determine the muscle fiber type predominance. Vc values will be low in endurance athletes with a high percentage of type I fibers and, on the other side, it will be high in athletes with explosive activity and a high percentage of type II or fast-twitch fibers [3,12].

MYOMETRY

The Myometry (MMT) is a non-invasive tool which assesses the viscoelastic muscle, fascia and connective tissue properties (either in the tension or rest state), [23]. It has a good reliability observed by different studies among healthy and injured population [24-29] and has shown an excellent test-rest reliability (ICC = 0.80-0.93) [30,31]. The MMT is placed

perpendicular to the structure and the device automatically performs a series of impulses (Figure 3). The tissue responds to the mechanical stimulus by damped oscillations that are recorded by an acceleration sensor and processed by an internal microprocessor. Following parameters are obtained using this oscillations average value (Figure 4 and Table 1).



Figure 3: MMT procedure.

Muscle tone (Hz)

It is defined as the muscle intrinsic tension at cellular level in a rest state. In cases of high muscle tone, correct blood supply is restricted, which causes earlier muscle fatigue and it could delay the recovery [32].

Stiffness (N/m)

It is the biomechanical muscle property that characterizes the resistance to an external force that deforms its initial shape [33].

Elasticity

It is the biomechanical muscle property that characterizes the ability to recover its initial shape after the elimination of an external force that deforms it. The elasticity is calculated from the record of the amplitude decrease [32], and it represents the mechanical released energy during an oscillation cycle.

Relaxation (m/s)

Is the time for a muscle to recover its shape from after the removal of an external force (ms) [33].

Creep

It is the tissue gradual elongation over time when placed under a constant tensile stress [32,33].

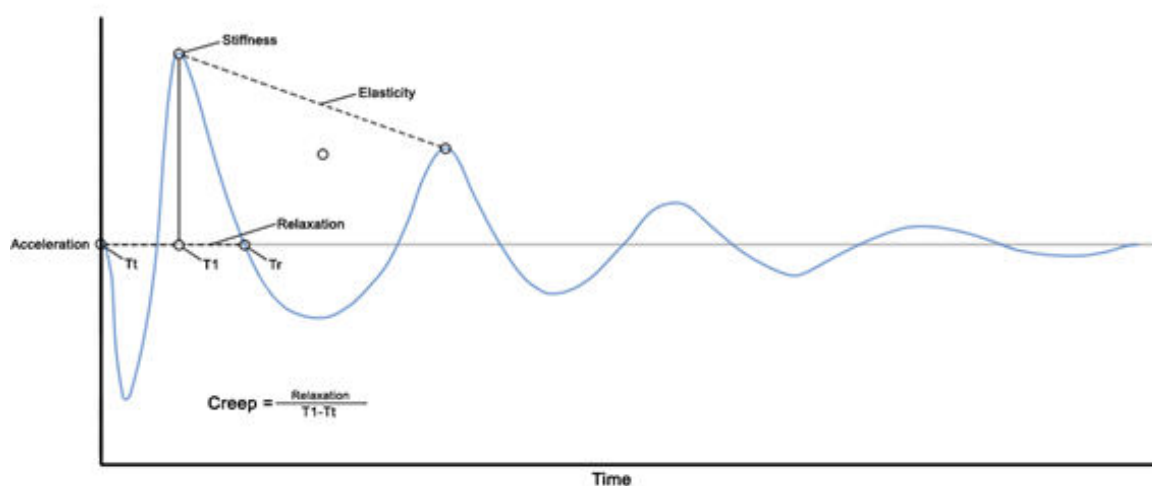


Figure 4: NMR response and MMT values.

Table 1: measures reliability

Outcome	Measuring instrument	Provided information	Reliability
Maximal Radial displacement (Dm)	Tensiomyography	Maximal radial displacement of the muscle contraction or its stiffness	0.97 a 0.86 0.98 [34] 0.98 [15] 0.98 [35] 0.97 [16] 0.86 [36] 0.92 [37] 0.95 [38,39]
Delay time (Td)	Tensiomyography	Time between an electrical impulse and 10% of the contraction	0.91 [34] 0.94 [15] 0.94 [35] 0.86 [16] 0.60 [36] 0.89 [37] 0.82 [38,39]
Contraction time (Tc)	Tensiomyography	Time between 10% and 90% of the contraction after an impulse	0.92 [34] 0.97 [15] 0.98 [35] 0.92 [16] 0.62 [36] 0.83 [37] 0.86 [38,39]
Sustained time (Ts)	Tensiomyography	Time between 50% of the contraction and 50% of the relaxation after an impulse	0.81 [34] 0.89 [15] 0.94 [35] 0.96 [16] 0.78 [36] 0.90 [37] 0.94 [38,39]
Relaxation time (Tr)	Tensiomyography	Time between 90% and 50% of the relaxation. It indicates muscular fatigue	0.42 [34] 0.86 [15] 0.88 [35] 0.77 [16] 0.79 [36] 0.88 [37] 0.78 [38,39]
Tone	Myometry	Intrinsic tension on the cellular level	0,91-0,96 [40,41]
Stiffness	Myometry	Resistance to a contraction or to an external force that deforms its initial shape	0,91-0,96 [40,41]
Elasticity	Myometry	Ability to recover the muscle initial shape after a contraction or removal of an external force of deformation	0,78-0,86 [40,41]
Relaxation time	Myometry	Time to recover the muscle initial shape after a contraction or removal of an external force of deformation	
Creep	Myometry	Ratio of deformation and relaxation time. Gradual elongation of a tissue over time when placed under a constant tensile stress.	

METHODOLOGICAL CONSIDERATIONS FOR THE NEUROMUSCULAR RESPONSE STUDY

Regarding the recommendations made by Rodríguez-Matoso et al., [42]. In order to do a correct NMR measurement, it is necessary to follow the next considerations:

1. To analyze only the musculature or subcutaneous fascial tissue. In people with large amounts of adipose tissue or deep muscles, measurement will not be feasible.
2. To state correctly the segments to be studied. Changes in the position will alter the measurement. So it is important to measure it always with the same subject position.

3. Accurate sensor placement. Although with the myometry the sensor placement could be different (depending on whether we want to analyze the fascia muscle), in the tensiomyography the sensor placement must be in the most prominent area of the muscle and in the middle of the electrodes that will cause the electrical contraction.

4. To avoid muscle tissue tetanization. In the case of using the TMG it is advisable to space the contraction discharges in order to avoid muscle tissue tetanization. If you want to use both tools, it is better to use firstly the myometry in order to avoid tone changes.

5. To avoid studying fatigued muscle, unless you want to analyze this muscle condition.
6. To check the ambient and segment temperature before the measurement. The NMR is a set of biomechanical and viscoelastic muscle properties so the temperatures changes could alter them.

CONCLUSION

The neuromuscular response is a set of parameters that allow us to assess the myofascial tissue state (fascia and muscle). These parameters can help both the physiotherapist and the physical trainer to know about this tissue state. It is important in order to prevent injuries and to plan training or treatments. Myometry (or myoton) and tensiomyography are two non-invasive tools that allow us to know about muscle properties with a good reliability. The principal strength of these two tools is that they are both cheaper than MRI and EMG activity. Moreover, they are easily transportable and small enough to facilitate his use. On the other hand, one important limitation of these two tools is that they did not take into account the subject willfulness. Future studies are necessary to know different treatments or training effects in the NMR.

REFERENCE

1. Sánchez-Ureña B, Rojas-Valverde D, Gutiérrez-Vargas R. (2018). Effectiveness of Two Cold Water Immersion Protocols on Neuromuscular Function Recovery. A Tensiomyography Study. *Frontiers in physiology*. 9: 766.
2. Vain A, Kums T. (2002). Criteria for preventing overtraining of the musculoskeletal system of gymnasts. *Biology of sport*. 19: 329-346.
3. Dahmane R, Valenčič V, Knez N, Eržen I. (2001). Evaluation of the ability to make non-invasive estimation of muscle contractile properties on the basis of the muscle belly response. *Medical and biological engineering and computing*. 39: 51-55.
4. Marusiak J, Jaskólska A, Budrewicz S, Koszewicz M, Jaskólski A. (2011). Increased muscle belly and tendon stiffness in patients with Parkinson's disease, as measured by myotonometry. *Mov Disor*. 26: 2119-2122.
5. Rätsep T, Asser T. (2011). Changes in viscoelastic properties of skeletal muscles induced by subthalamic stimulation in patients with Parkinson's disease. *Clin Biomech (Bristol, Avon)*. 26: 213-217.
6. Marusiak J, Jaskólska A, Koszewicz M, Budrewicz S, Jaskólski A. (2012). Myometry revealed medication-induced decrease in resting skeletal muscle stiffness in Parkinson's disease patients. *Clin Biomech (Bristol, Avon)*. 27: 632-635.
7. Gervasi M, Sisti D, Amatori S, Andrezza M, Benelli P, et al. (2017). Muscular viscoelastic characteristics of athletes participating in the European Master Indoor Athletics Championship. *Eur J Appl Physiol*. 117: 1739-1746.
8. Harber M, Crane J, Douglass M, Weindel K, Trappe T, et al. (2008). Resistance exercise reduces muscular substrates in women. *Int J Sports Med*. 29: 719-725.
9. Murray AM, Jones TW, Horobeanu C, Turner AP, Sproule J. (2016). Sixty Seconds of Foam Rolling does Not Affect Functional Flexibility Or Change Muscle Temperature in Adolescent Athletes. *Int J Sports Phys Ther*. 11: 765-776.
10. Valenčič V. (1990). Direct measurement of the skeletal muscle tonus. *Advances in external control of human extremities. Beograd Nauka*. 102-108.
11. Valenčič V, Knez N. (1997). Measuring of skeletal muscles' dynamic properties. *Artif Organs*. 21: 240-242.
12. Dahmane R, Djordjević S, Šimunič B, Valenčič V. (2005). Spatial fiber type distribution in normal human muscle: histochemical and tensiomyographical evaluation. *J Biomech*. 38: 2451-2459.
13. Carrasco L, Sanudo B, de Hoyo M, Pradas F, Da Silva ME. (2011). Effectiveness of low-frequency vibration recovery method on blood lactate removal, muscle contractile properties and on time to exhaustion during cycling at VO₂max power output. *Eur J Appl Physiol*. 111: 2271-2279.
14. Rodríguez-Matoso D, Rodríguez-Ruiz D, S Sarmiento, Vaamonde D, Silva-Grigoletto ME, et al. (2010). Reproducibility of muscle response measurements using tensiomyography in a range of positions. *Revista Andaluza de Medicina del Deporte*. 3: 81-86.
15. Križaj D, Šimunič B, Žagar T. (2008). Short-term repeatability of parameters extracted from radial displacement of muscle belly. *Journal of Electromyography and Kinesiology*. 18: 645-651.
16. Tous-Fajardo J, Moras G, Rodríguez-Jiménez S, Usach R, Doutres DM, et al. (2010). Inter-rater reliability of muscle contractile property measurements using non-invasive

- tensiomyography. *Journal of Electromyography and Kinesiology*. 20: 761-766.
17. The tensiomyography at the service of the athlete. Workshop II Congress In-c D. The tensiomyography at the service of the athlete. Workshop II Congress In-D. The tensiomyography at the service of the athlete. Workshop II International University Congress on Health Sciences and Sports. Madrid: San Pablo CUE University; 2003
 18. Rusu L, Calina ML, Avramescu ET, Paun E, Vasilescu M. (2009). Neuromuscular investigation in diabetic polyneuropathy. *Romanian Journal of Morphol Embryol*. 50: 283-290.
 19. Rodríguez-Ruiz D, Quiroga M, Rodríguez-Matoso D, Sarmiento S, Losa J, et al. (2009). Aplicación de la tensiomiografía (TMG) en jugadores de vóley-playa. Estudio de caso. (p. 121-130). *Investigando para innovar en la actividad física y el deporte*. Vitoria: editores. Gidekit.
 20. Dahmane R, Valenčič V, Knez N, Eržen I. (2001). Evaluation of the ability to make non-invasive estimation of muscle contractile properties on the basis of the muscle belly response. *Med bio Eng comput*. 39: 51-55.
 21. Valencic V, Knez N, Simunic B. (2001). Tensiomyography: detection of skeletal muscle response by means of radial muscle belly displacement. *Biomed Eng*. 1: 1-10.
 22. Dahmane R, Djordjevič S, Šimunič B, Valenčič V. (2005). Spatial fiber type distribution in normal human muscle: histochemical and tensiomyographical evaluation. *J Biomech*. 38: 2451-2459.
 23. Aird L, Samuel D, Stokes M. (2012). Quadriceps muscle tone, elasticity and stiffness in older males: reliability and symmetry using the MyotonPRO. *Arch Gerontol Geriatr*. 55: 31-39.
 24. Bizzini M, Mannion AF. (2003). Reliability of a new, hand-held device for assessing skeletal muscle stiffness. *Clin Biomech (Bristol, Avon)*. 18: 459-461.
 25. Viir R, Laiho K, Kramarenko J, Mikkelsson M. (2006). Repeatability of trapezius muscle tone assessment by a myometric method. *Journal of Mechanics in Medicine and Biology*. 6: 215-228.
 26. Ditroilo M, Hunter AM, Haslam S, De Vito G. (2011). The effectiveness of two novel techniques in establishing the mechanical and contractile responses of biceps femoris. *Physiol Meas*. 32: 1315-1326.
 27. Chuang L, Wu C, Lin K. (2012). Reliability, validity, and responsiveness of myotonometric measurement of muscle tone, elasticity, and stiffness in patients with stroke. *Arch Phys Med Rehabil*. 93: 532-540.
 28. Agyapong-Badu S, Aird L, Bailey L, Mooney K, Mullix J, et al. (2013). Interrater reliability of muscle tone, stiffness and elasticity measurements of rectus femoris and biceps brachii in healthy young and older males. *Work Pap. Health Sci*. 1: 1-11.
 29. Davidson MJ, Bryant AL, Bower WF, Frawley HC. (2017). Myotonometry reliably measures muscle stiffness in the thenar and perineal muscles. *Physiotherapy Canada*. 69: 104-112.
 30. Bizzini M, Mannion AF. (2003). Reliability of a new, hand-held device for assessing skeletal muscle stiffness. *Clin Biomech (Bristol, Avon)*. 18: 459-461.
 31. Kelly JP, Koppenhaver SL, Michener LA, Proulx L, Bisagni F, et al. (2018). Characterization of tissue stiffness of the infraspinatus, erector spinae, and gastrocnemius muscle using ultrasound shear wave elastography and superficial mechanical deformation. *J Electromyography Kinesiol*. 38: 73-80.
 32. Chuang L, Wu C, Lin K. (2012). Reliability, validity, and responsiveness of myotonometric measurement of muscle tone, elasticity, and stiffness in patients with stroke. *Arch Phys Med Rehabil*. 93: 532-540.
 33. Zinder SM, Padua DA. (2011). Reliability, validity, and precision of a handheld myometer for assessing in vivo muscle stiffness. *J Sport Rehab*. 20.
 34. Jiménez AB, Roldán KF, Doblás JMM, Castro JAR. (2013). Reliability of tensiomyography (tmg) as a muscle assessment tool. *International Journal of Medicine and Sciences of Physical Activity and Sports*. 52: 647-656
 35. Šimunič B. (2012). Between-day reliability of a method for non-invasive estimation of muscle composition. *J electromyography kinesiol*. 22: 527-530.
 36. Ditroilo M, Smith IJ, Fairweather MM, Hunter AM. (2013). Long-term stability of tensiomyography measured under different muscle conditions. *Journal of Electromyography and Kinesiology*. 23: 558-563.

37. Carrasco Paez L, Sañudo Corrales, Francisco de Borja, Hoyo Lora Md, Ochiana G. (2011). Tensiomyographic characteristics of Rectus Femoris after a single bout of intense exercise. *Journal of Social Sciences*. 7: 354-357.
38. Rey E, Lago-Peñas C, Lago-Ballesteros J. (2012). Tensiomyography of selected lower-limb muscles in professional soccer players. *J Electromyography Kinesiology*. 22: 866-872.
39. Rey E, Lago-Peñas C, Lago-Ballesteros J, Casáis L. (2012). The effect of recovery strategies on contractile properties using tensiomyography and perceived muscle soreness in professional soccer players. *J Strength Cond Res*. 26: 3081-3088.
40. Nogales Espert A. (2004). Approach to the history of autopsies: I. Ancient civilizations. *Medicina Hippocratic School of Alexandria. Galen. EJ Autopsy*. 3-8.
41. Lohr C, Braumann K, Reer R, Schroeder J, Schmidt T. (2018). Reliability of tensiomyography and myotonometry in detecting mechanical and contractile characteristics of the lumbar erector spinae in healthy volunteers. *Eur J Appl Physiol*. 118: 1349-1359.
42. Rodríguez-Matoso D, García-Manso J, Sarmiento S, De Saa Y, Vaamonde D, et al. (2012). Evaluation of muscle response as a control tool in the field of physical activity, health and sports. Assessment of muscle response as a control tool in the area of physical activity, health, and sports. *Andalusian Journal of Sports Medicine*. 5: 28-40.